

Mepitel® One

New wound contact layer with Safetac® technology


Polyurethane net

- Open mesh structure allows free transfer of wound exudate to outer absorbent dressing and delivery of topical preparations to the wound¹¹⁻¹³
- Highly transparent
- Thin and conformable for optimal patient comfort and secure adhesion

Safetac® layer (soft silicone)

- Reduces pain and trauma before, at and after dressing change⁹
- Seals around the wound margins to reduce risk of maceration¹⁰
- Adheres gently to dry intact skin but not to the moist wound bed

Safetac
TECHNOLOGY

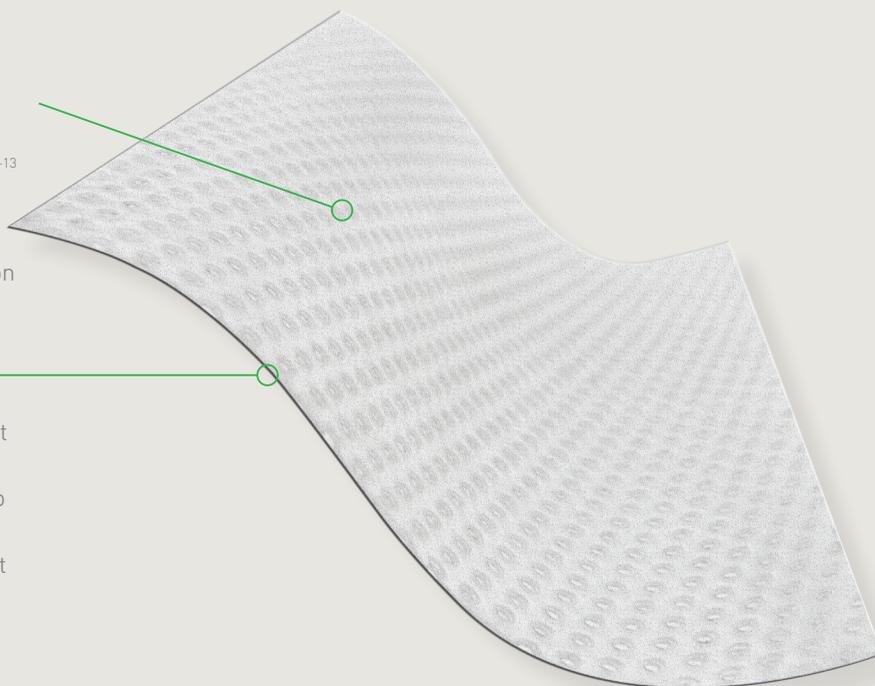

- Minimizes pain and trauma at dressing changes^{1,2}
- Can remain in place for up to 14 days³⁻⁷ which allows cost-effective^{1,8} and undisturbed wound healing
- Non-adherent outer surface for optimal conformability, flexibility and ease of application

Proven choice for a better outcome

Safetac*, pioneered by Mölnlycke, delivers above and beyond the ordinary. Proven to help optimize the wound healing journey and even prevent wounds, dressings with Safetac are the safe choice for patients and a champion for higher standards in wound care.

In fact, we have a wealth of evidence that supports the clinical and economic benefits of dressings with Safetac, including Mepilex®, Mepitel®, Mepiform® and Mepitac®. To date, these dressings have helped millions of patients worldwide⁷⁻⁹.


* A unique proprietary technology exclusive to Mölnlycke Health Care

Safetac
TECHNOLOGY


Mepitel® One


Mölnlycke®


Directions for use

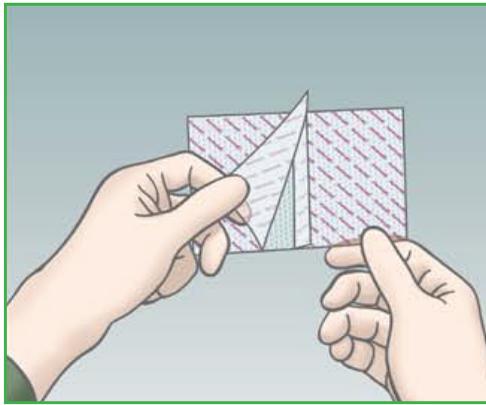

Gently clean the wound area; dry surrounding skin. Remove the release film.

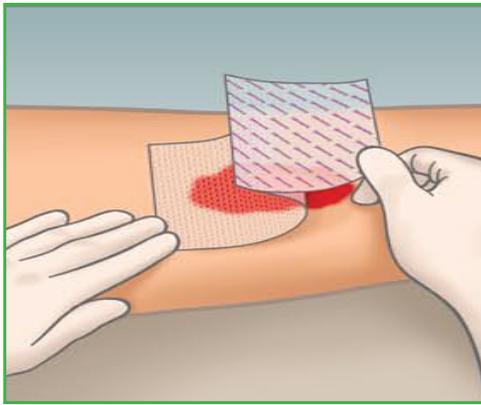

Apply Mepitel One to the wound allowing it to overlap onto the surrounding skin by 2 cm.

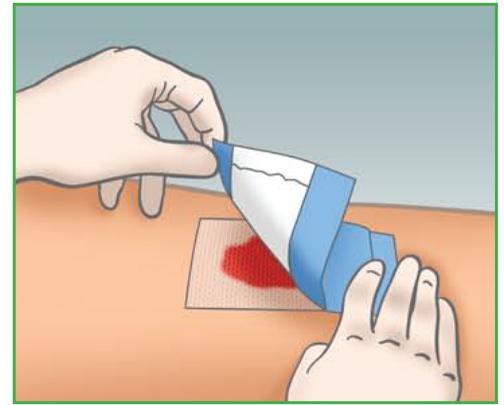

Apply an outer absorbent dressing such as Mesorb and fixate in place.

How Mepitel One works

Mepitel One can be left in place for up to 14 days³⁻⁷, depending on the condition of the wound. The porous structure of Mepitel One allows exudate to pass into an outer absorbent dressing. The Safetac wound contact surface protects the wound and peri-wound area and prevents the outer dressing from sticking to the wound. The Safetac layer also seals around the wound edges, preventing leakage of exudate onto the surrounding skin, thus minimizing the risk of maceration. Mepitel One is thin, transparent and has a smooth, non-adherent outer surface for optimal conformability, flexibility and ease of use.

Benefits of Mepitel

- Minimizes pain and trauma at dressing changes.
- Can remain in place for up to 14 days which in turn ensures undisturbed wound healing
- Minimizes the risk of maceration
- Maintains integrity over time; does not dry out and leaves no residue on removal
- Transparent for easy wound inspection during application and during wear
- Conforms well to body contours, promoting patient comfort during wear and secure adhesion

Indications for use

Mepitel One is designed for a wide range of wounds such as skin tears, skin abrasions, surgical incisions, partial thickness burns, traumatic wounds, blistering, lacerations, partial and full thickness grafts, radiation skin reactions, leg and foot ulcers. It can also be used as a protective layer on non-exuding wounds and on areas with fragile skin.

Mepitel® One Assortment (Sterile packed)

Art. no	Size cm	Pcs/Box	Pcs/Case
289100	5 × 7.5	10	70
289300	7.5 × 10	10	40
289500	10 × 18	10	70
289700	17 × 25	5	40
289750	27.5 × 50	2	14

Precautions

- When used on bleeding wounds or wounds with viscous exudate, Mepitel One should be covered with a moist outer dressing until hemostasis is achieved or the exudate becomes less viscous.
- When Mepitel One is used for the fixation of skin grafts, the dressing should not be changed before the fifth day post application.

Warnings

- Mepitel One has a higher adhesion level than Mepitel. When using Mepitel One on Epidermolysis Bullosa patients, use caution and surveillance at dressing changes.
- When Mepitel One is used on burns treated with meshed grafts, avoid placing unnecessary pressure upon the dressing. Imprints can occur if the product is not used properly.
- When Mepitel One is used after facial resurfacing, avoid placing unnecessary pressure upon the dressing and lift and reposition the dressing at least every second day. Imprints can occur if the product is not used properly.

References:

1. Gotschall CS, et al. Prospective, randomized study of the efficacy of Mepitel on children with partial-thickness scalds. *Journal of Burn Care & Rehabilitation* 1998;19(4):279-283.
2. Bugmann Ph, et al. A silicone-coated nylon dressing reduces healing time in burned paediatric patients in comparison with standard sulfadiazine treatment: a prospective randomized trial. *Burns* 1998;24:609-612.
3. Eagle M. Use of non-adherent silicone dressing Mepitel to meet client centered needs in chronic non-healing wounds. *Clinical Report Mölnlycke Health Care* [1998].
4. Taylor R. Use of a silicone net dressing in severe mycosis fungoides. *JoWC*, Vol 8, No 9 [1999], p.429-430.
5. Young T. Fungating wounds: their diagnosis and management. *Community nurse*, 5, No 10 [1999], p. 53-54.
6. Marconi R, Laverda F, Trevisan G. Poster Presentation European Wound Management Association, Helsinki, Finland, 2009.
7. Barrazoli R, Fracalenta E, Schiavon M. Poster Presentation European Wound Management Association, Helsinki, Finland, 2009.
8. Rippon M, Davies P, White R, Bosanquet N. Cost implications of using an atraumatic dressing in the treatment of acute wounds. *JoWC*, vol 17, No 5 [2008], p. 224-7.
9. Dykes PJ et al. Effects of adhesive dressings on the stratum corneum of the skin. *J Wound Care* 2001; 10(2):7-10.
10. Dykes PJ. The effect of adhesive dressing edges on cutaneous irritation and skin barrier function. *J Wound Care* 2007; 16(3):97-100.
11. Dahlstrom KK, Scand J *Plast Reconstr Surg Hand Surg* 1995;29(4):325-7.
12. Vloemans AFP, Kreis RW. *Scandinavian Journal of Plastic and Reconstructive Hand Surgery* 1994;28:75-6.
13. Lapioli-Zufelt A, Morris EJ. *Journal of Wound, Ostomy and Continence Nursing* 1998;25(6):314-6.

Mölnlycke
1-800-494-5134
www.molnlycke.ca

Mölnlycke Health Care AB, Box 13080, SE-40252 Göteborg, Sweden.
Phone +46317223000. The Mölnlycke Health Care, Mepitel®One, and Safetac® names and respective logos are registered globally to one or more of the Mölnlycke Health Care Group of Companies.
© 2017 Mölnlycke Health Care AB. All rights reserved.




Mölnlycke®

CEWC00601707